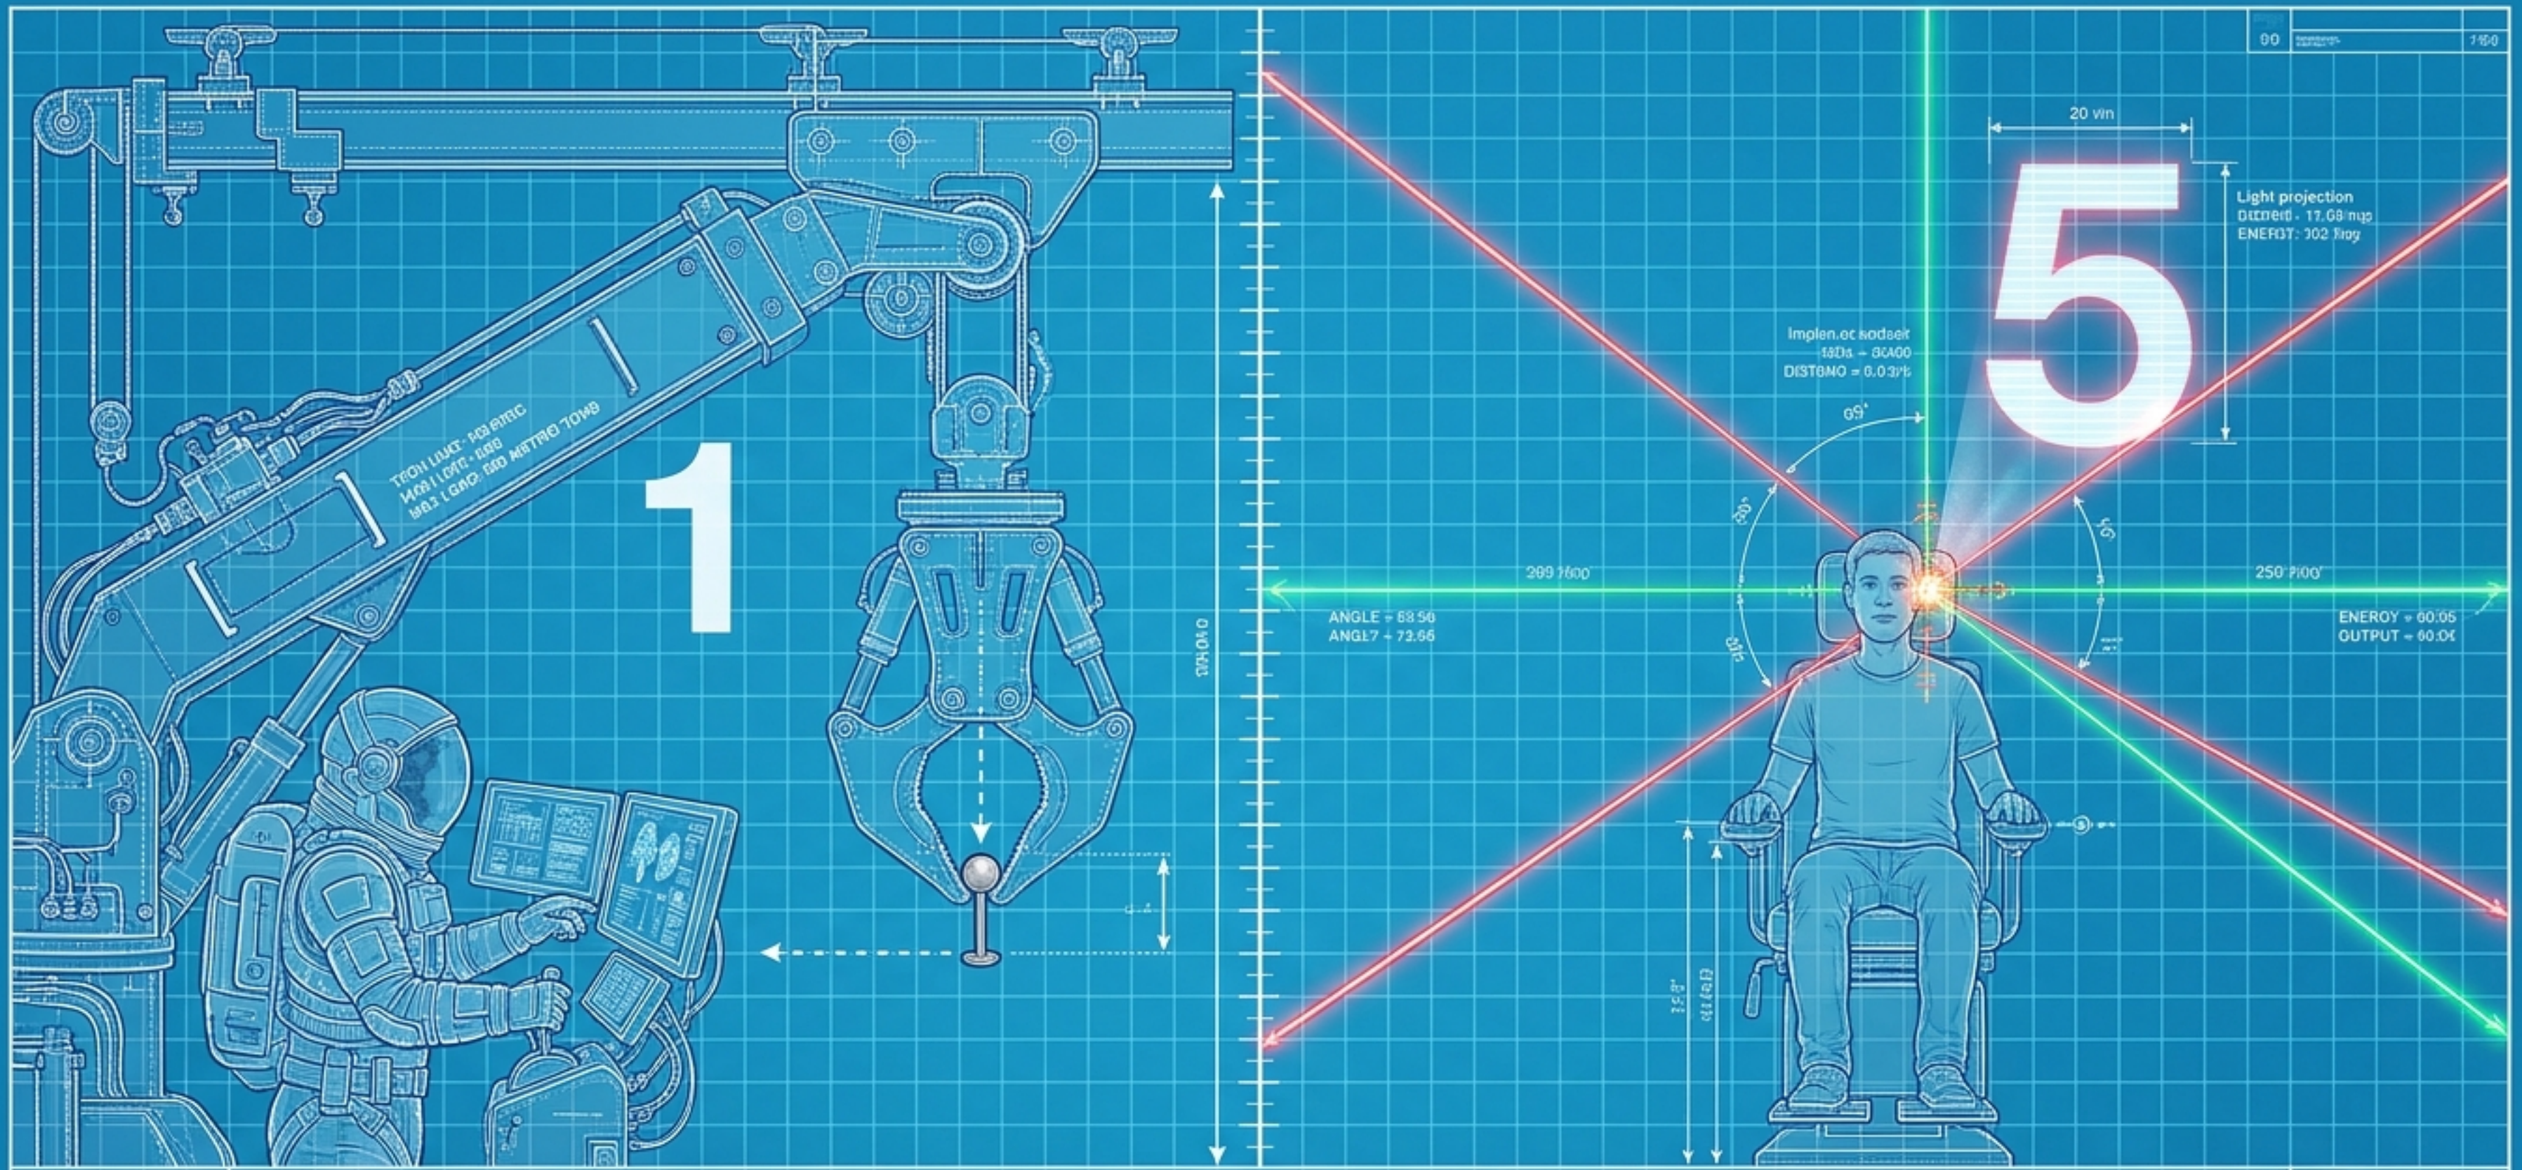


Medical implant infection rates range from 1 to 5% for primary procedures.

The orbital laser alignment array definitely justifies the tip.