


DO USE NATURAL TISSUE ELASTICITY.

DEAD STRETCHING USES JEWELLERY WEIGHT.

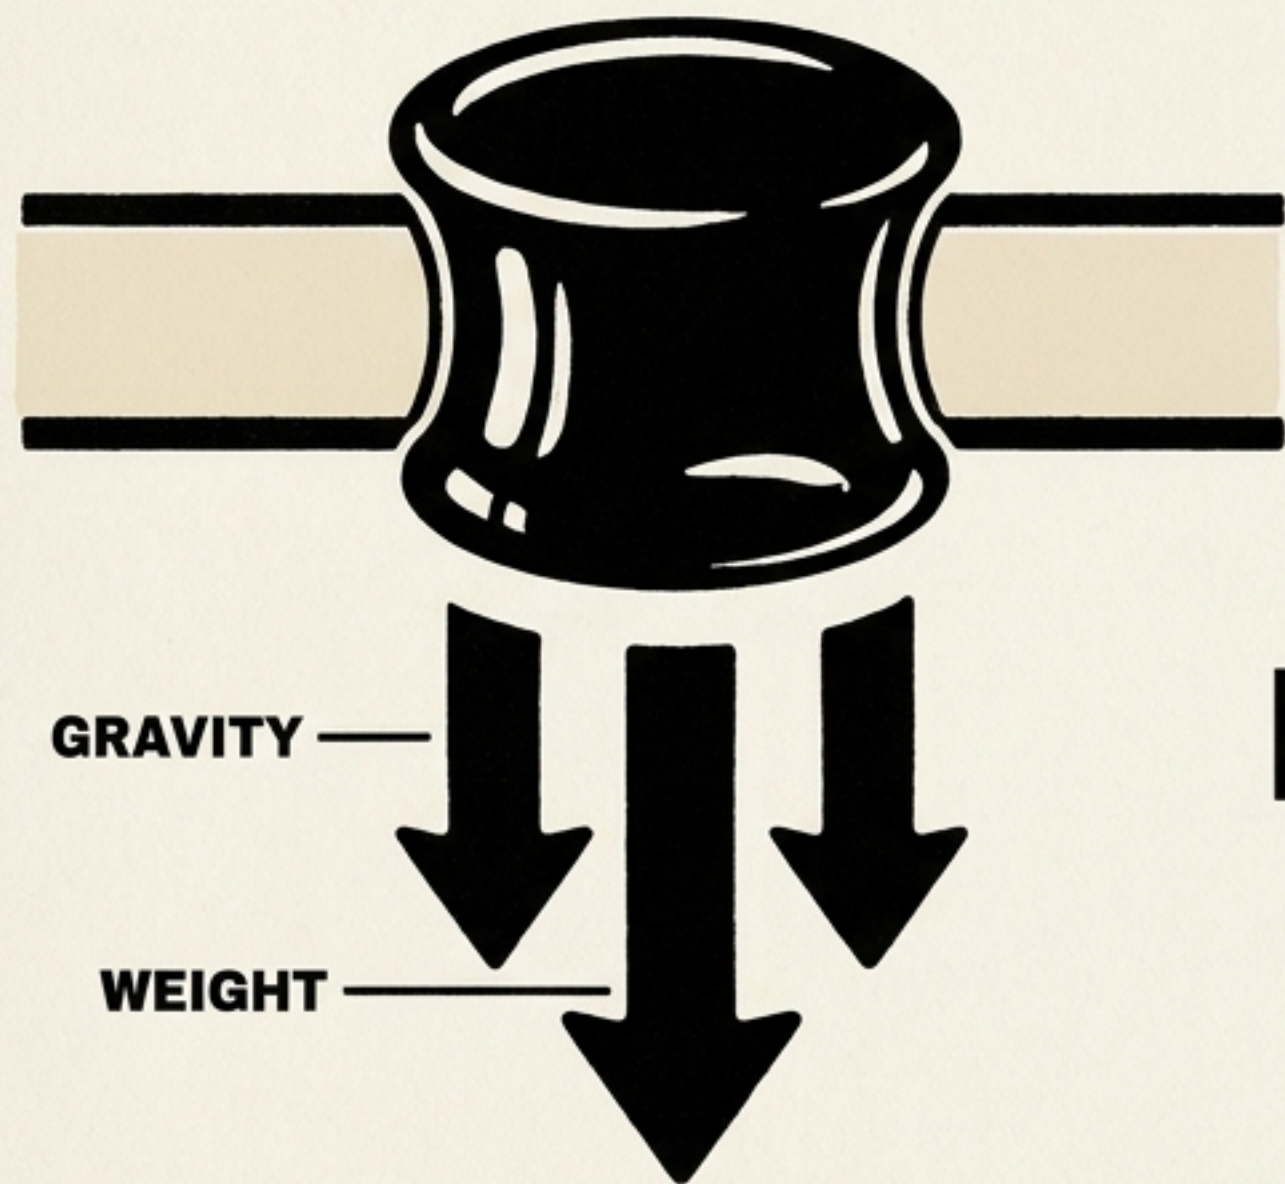


**FORCED DIAMETER
INCREASES PUSH
LINING OUTWARD.**

**INTERMEDIATE SIZES
REDUCE RISK BY
80 PERCENT.**

DO NOT USE INSERTION TAPERS.

TAPERS APPLY DANGEROUS ASYMMETRIC PRESSURE.

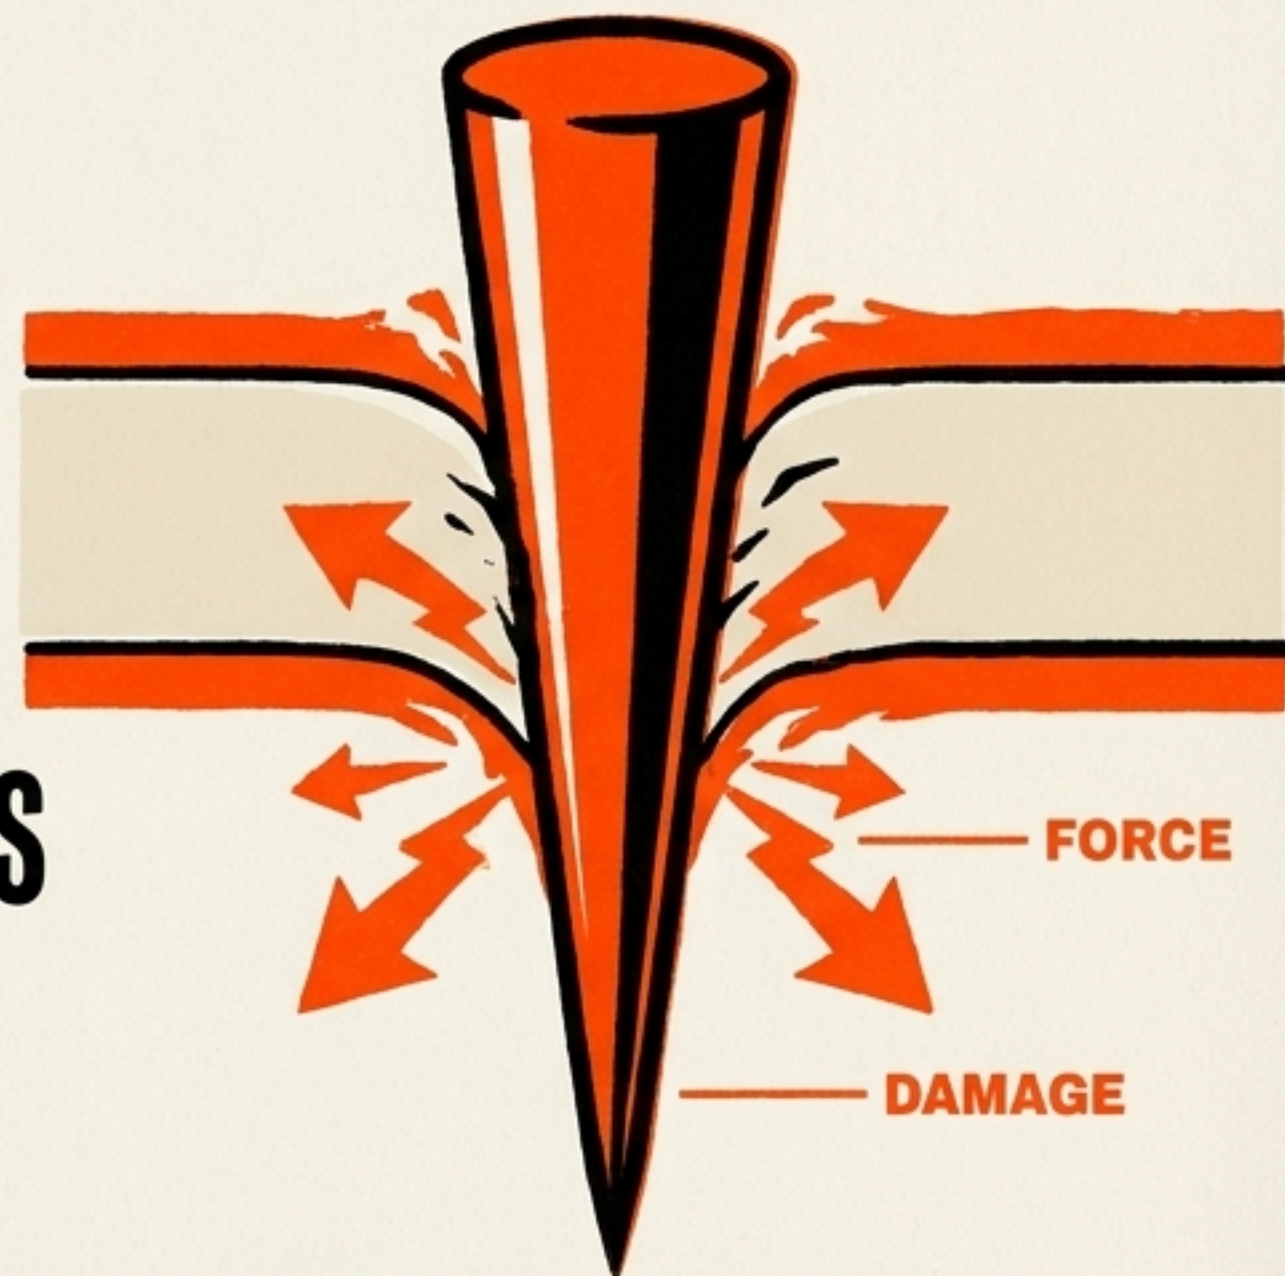

**INSERTION GUIDES MUST NEVER ACT AS FORCED TISSUE STRETCHING INSTRUMENTS.
DEAD STRETCHING IS THE SAFER METHOD.**