


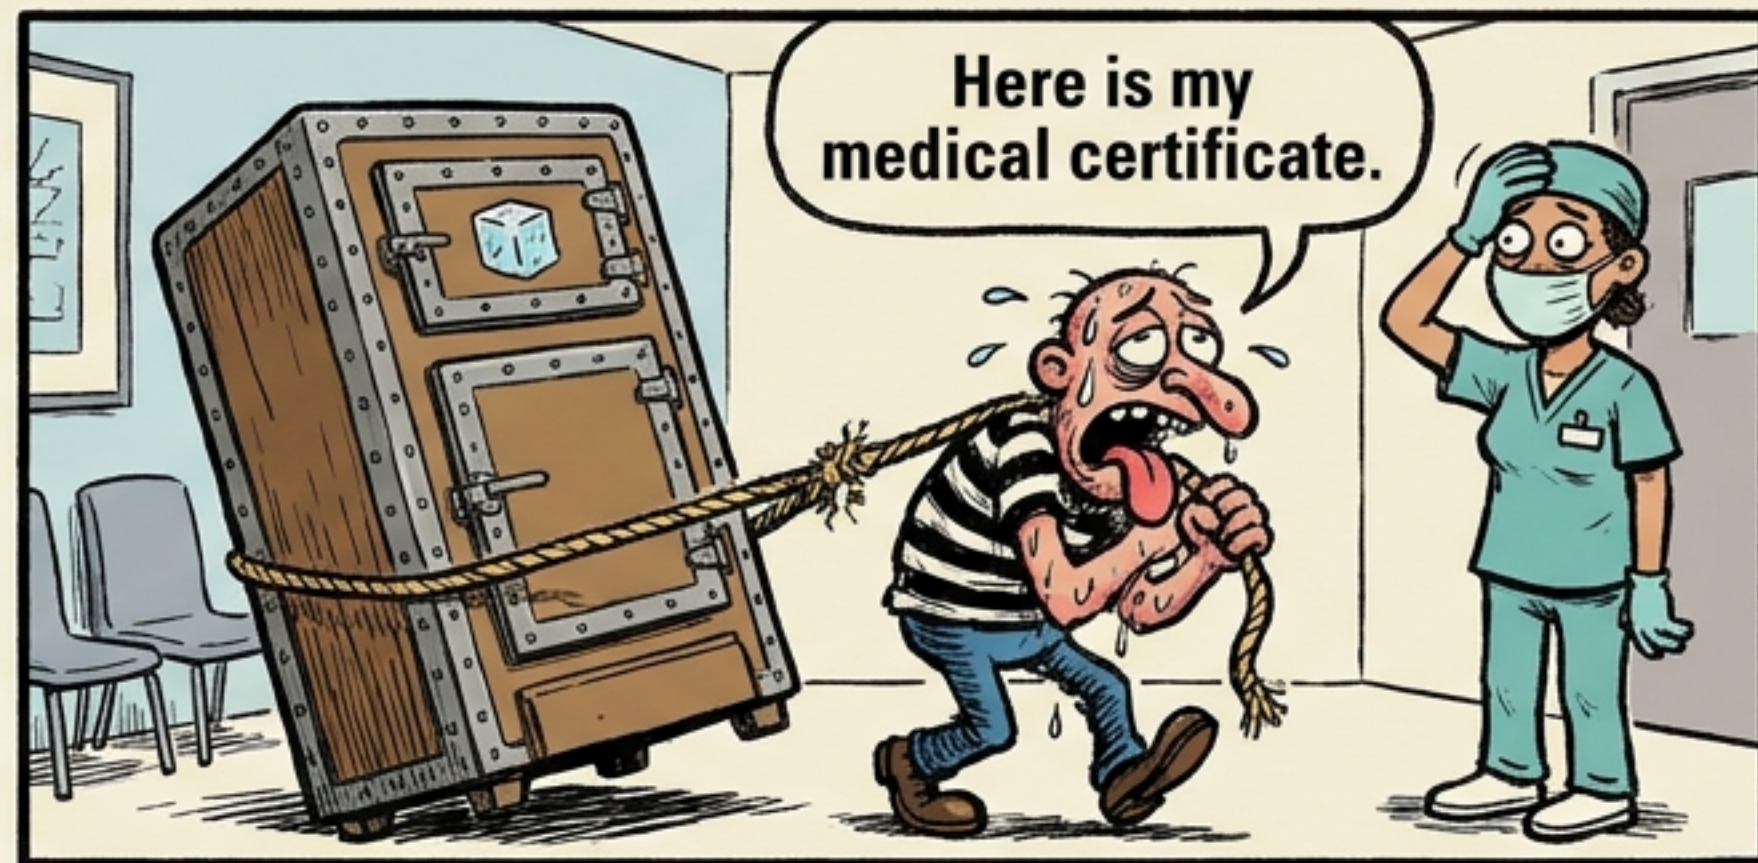

Cold-working creates ferromagnetic phases in surgical steel, making the household magnet test completely unreliable.

An icebox is not a valid medical certificate.