


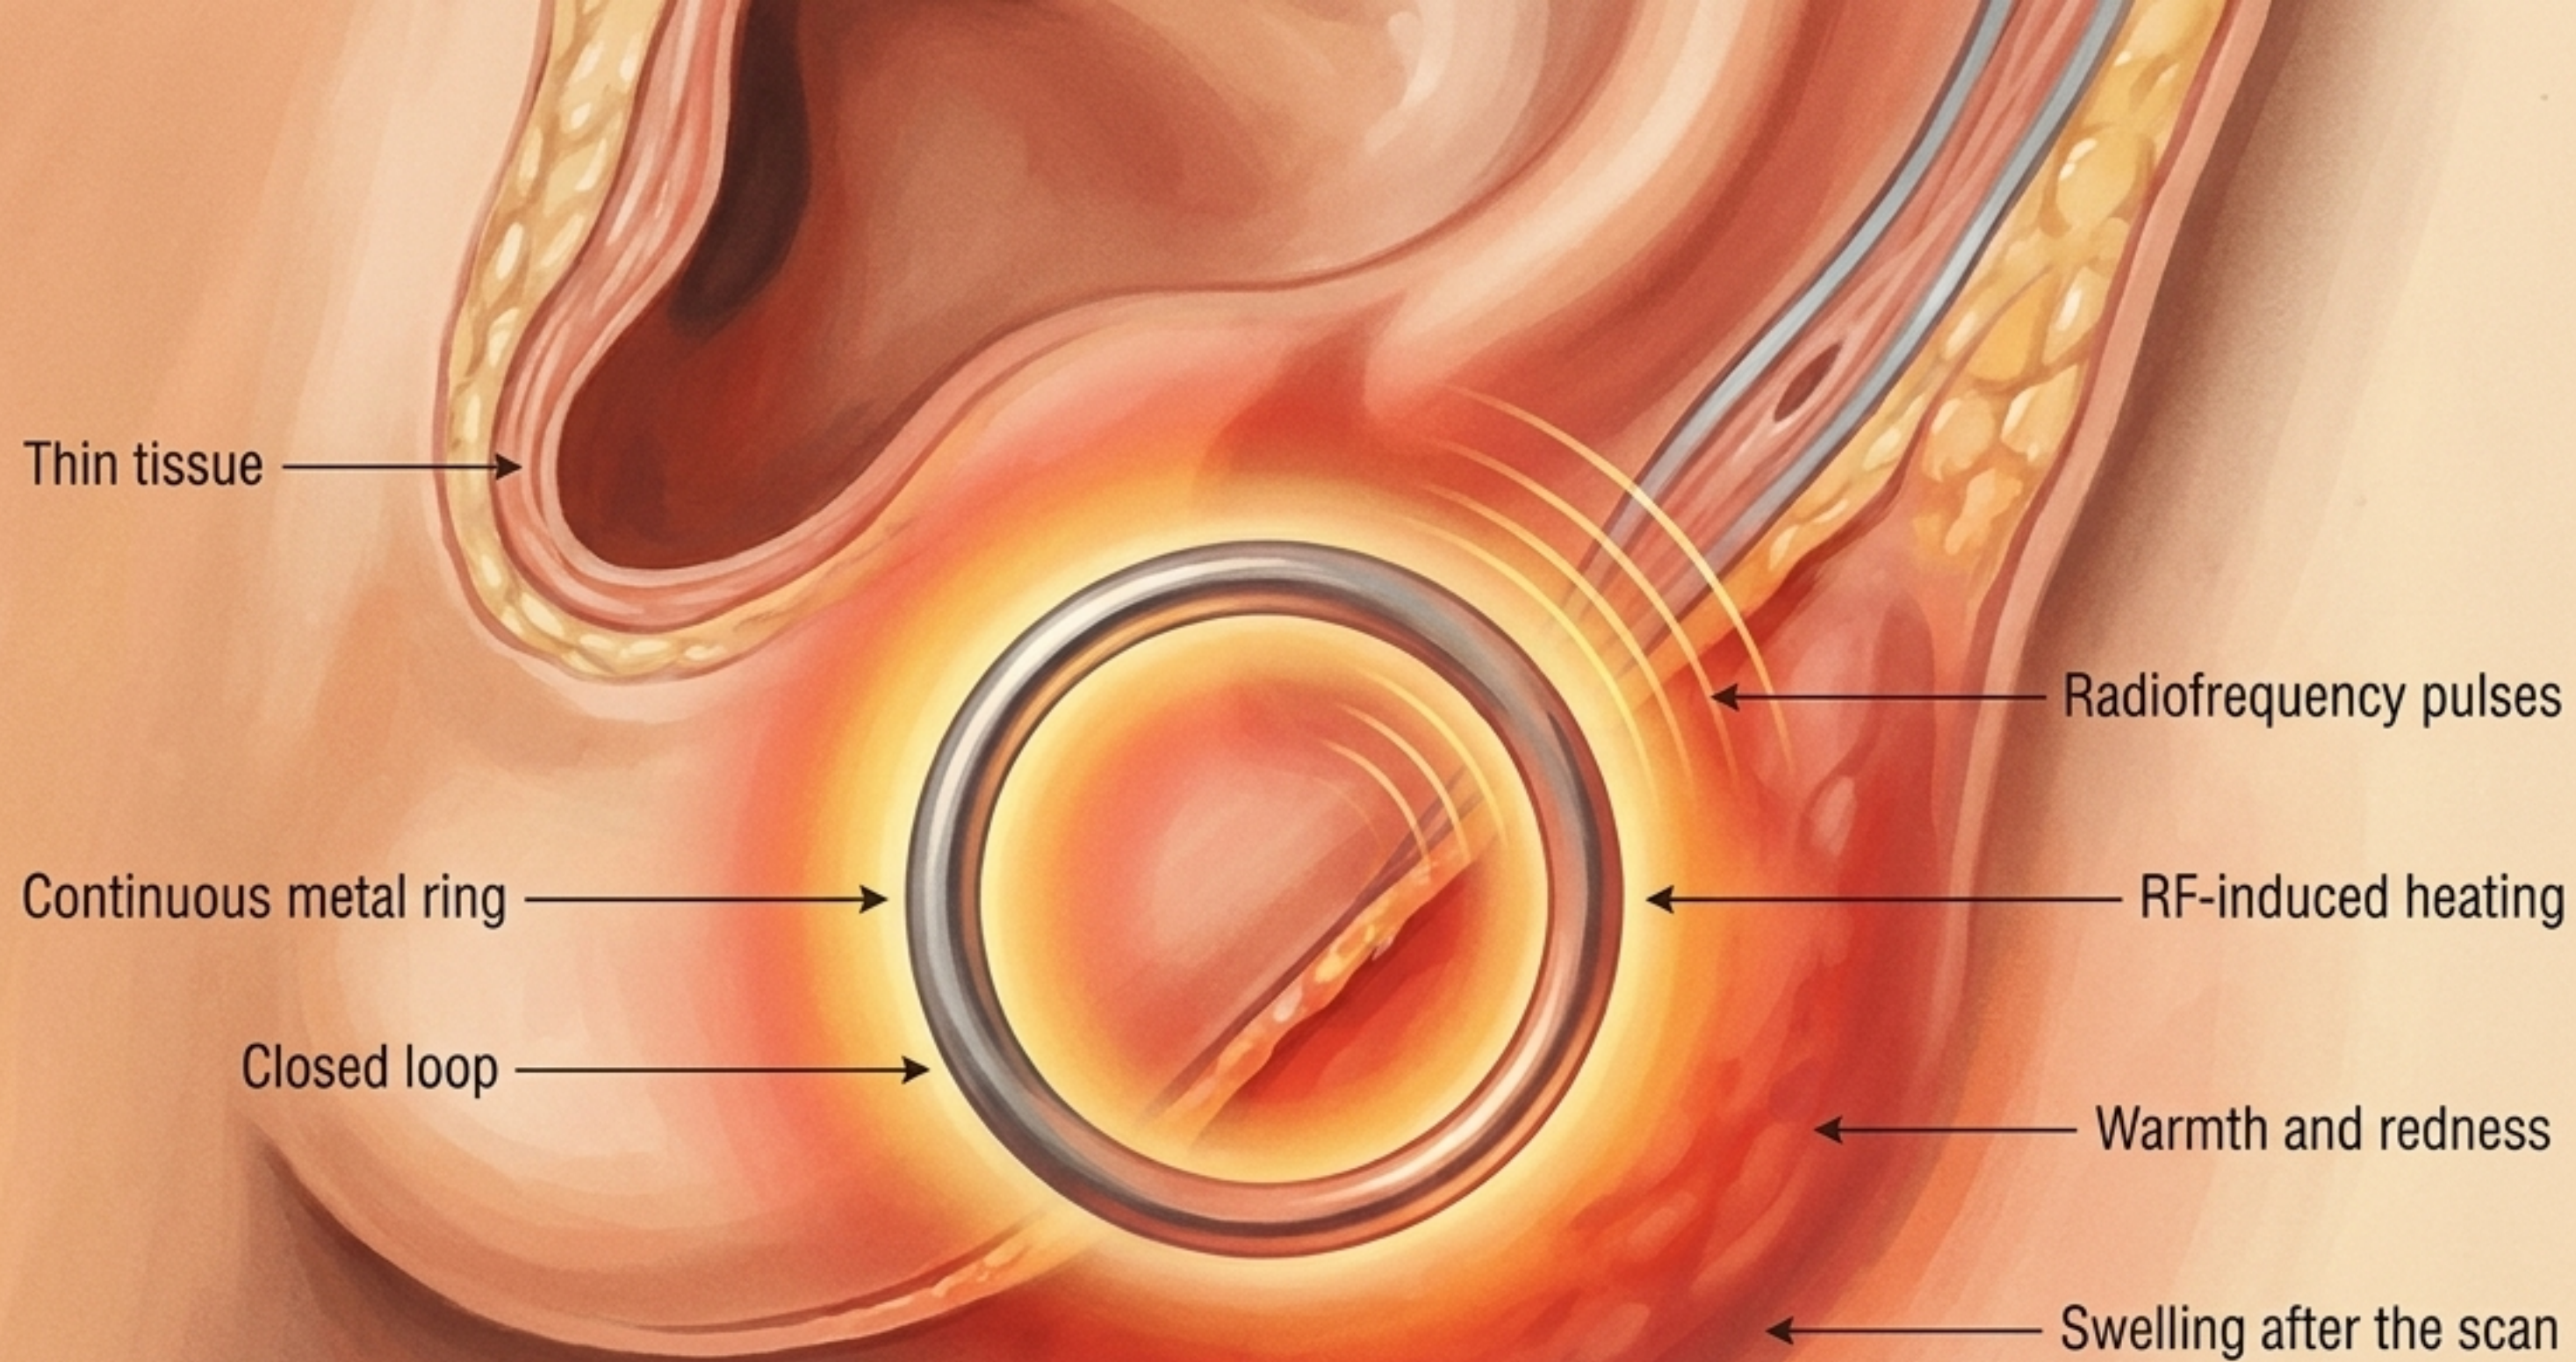

The scanner's radiofrequency pulses induce continuous electrical currents in conductive metal rings, causing significant tissue heating over time.

Swap closed hoops for straight barbells.