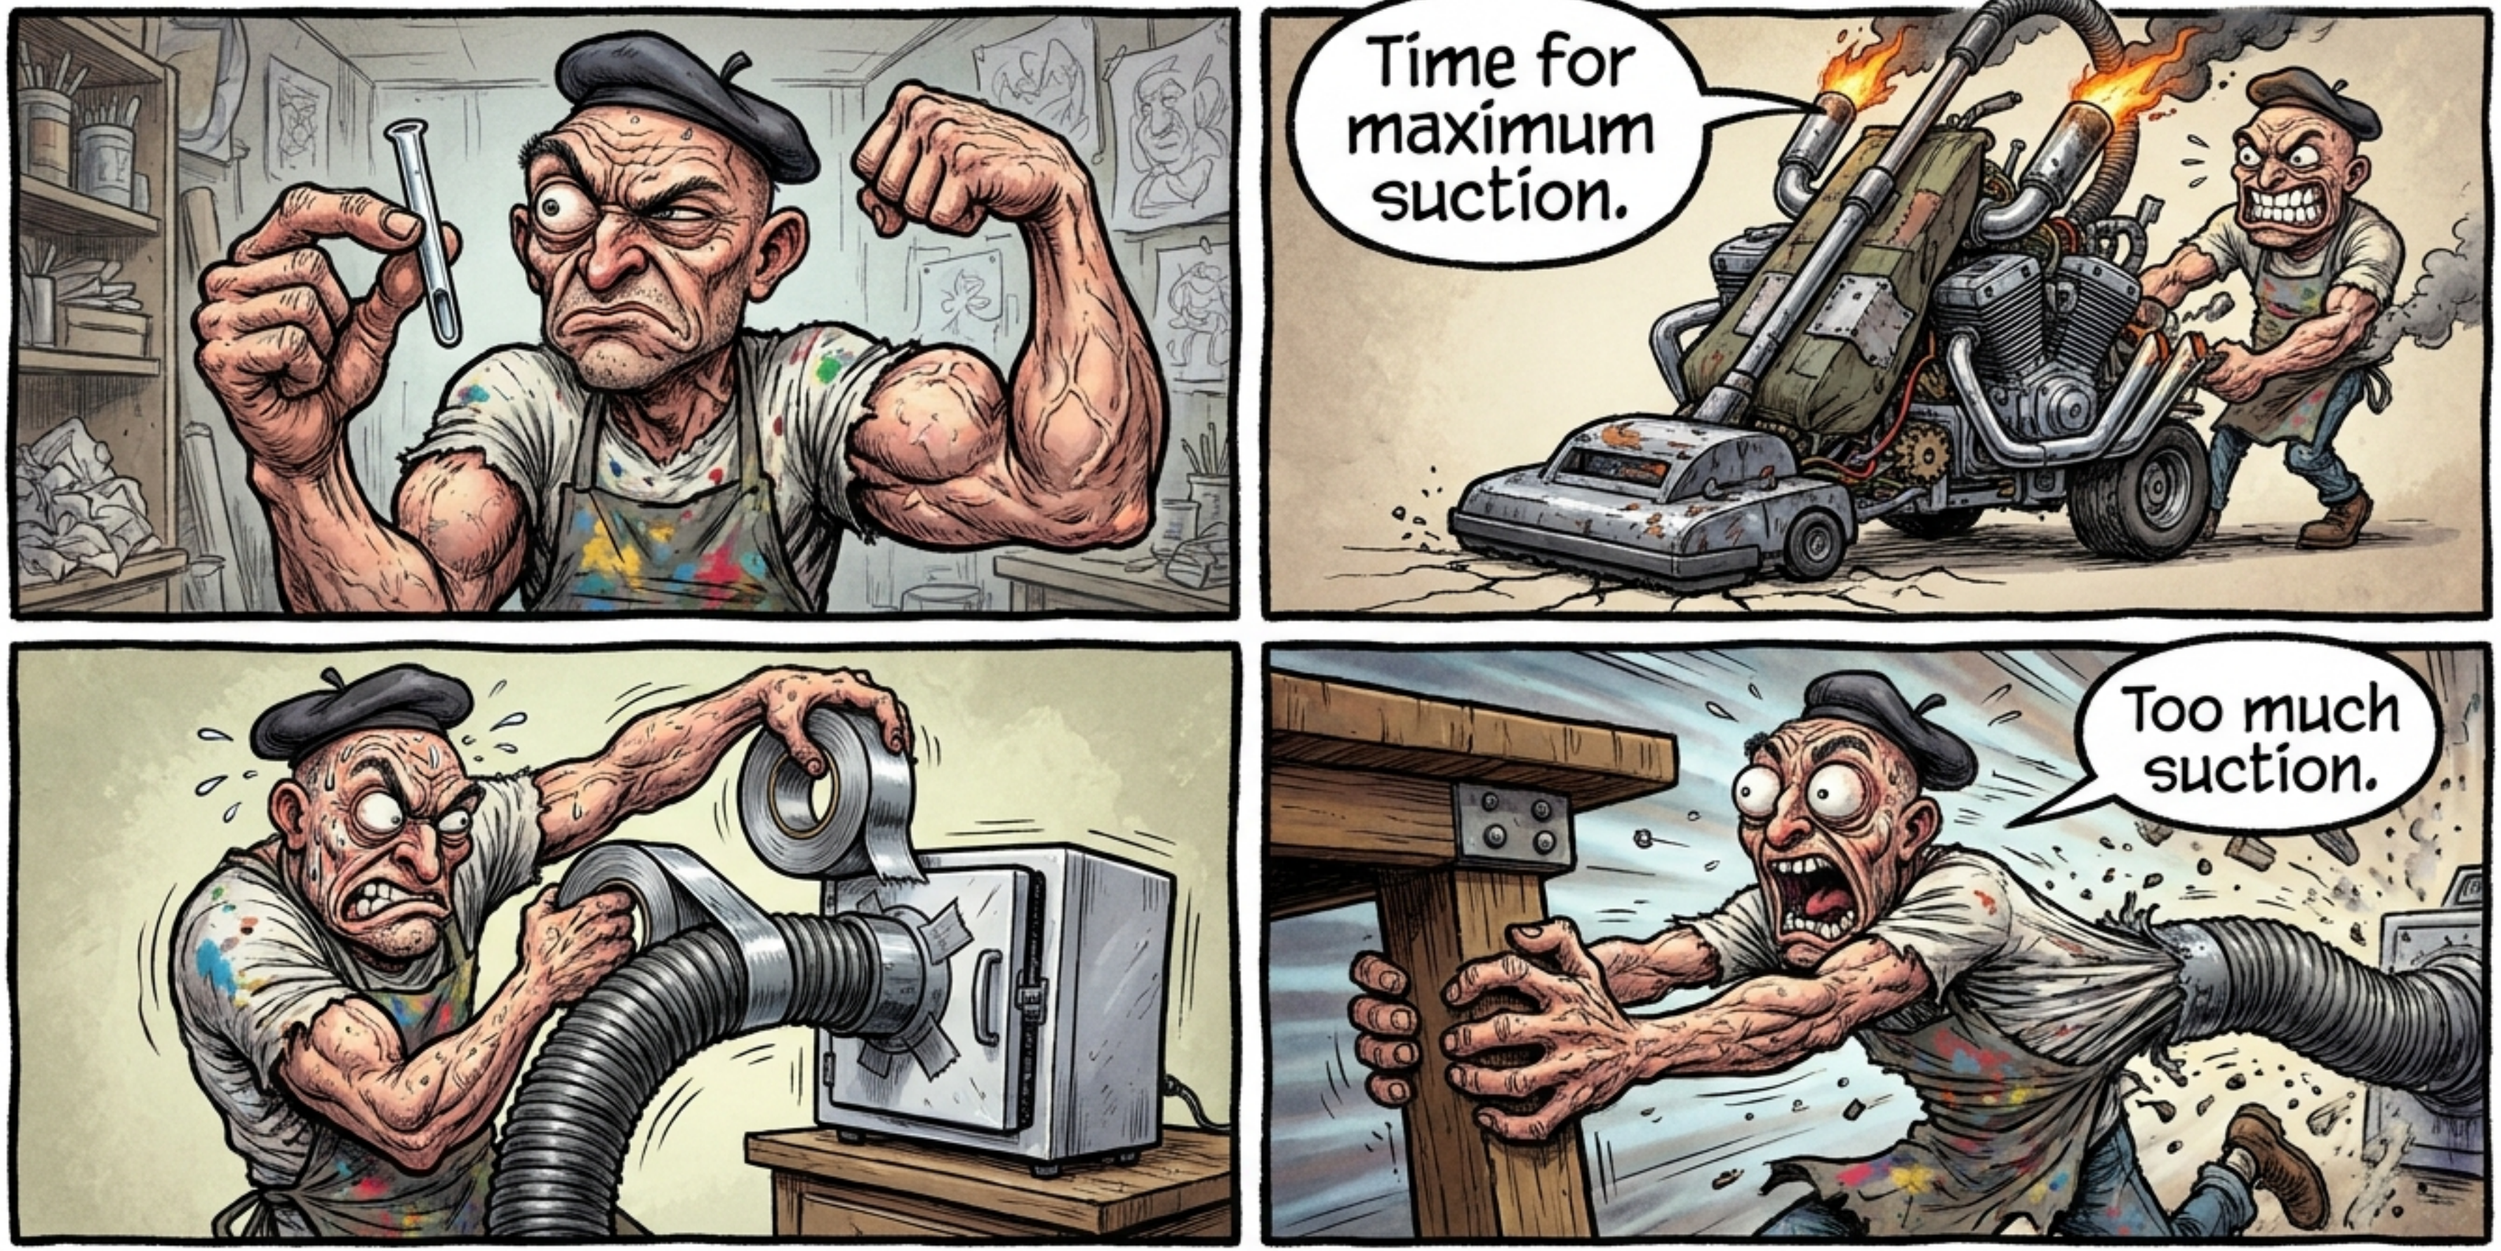


VACUUM AUTOCLAVES ARE THE RECOMMENDED STANDARD FOR STERILISING WRAPPED AND HOLLOW INSTRUMENTS. HOUSEHOLD APPLIANCES LACK THE REQUIRED SUBTLETY.