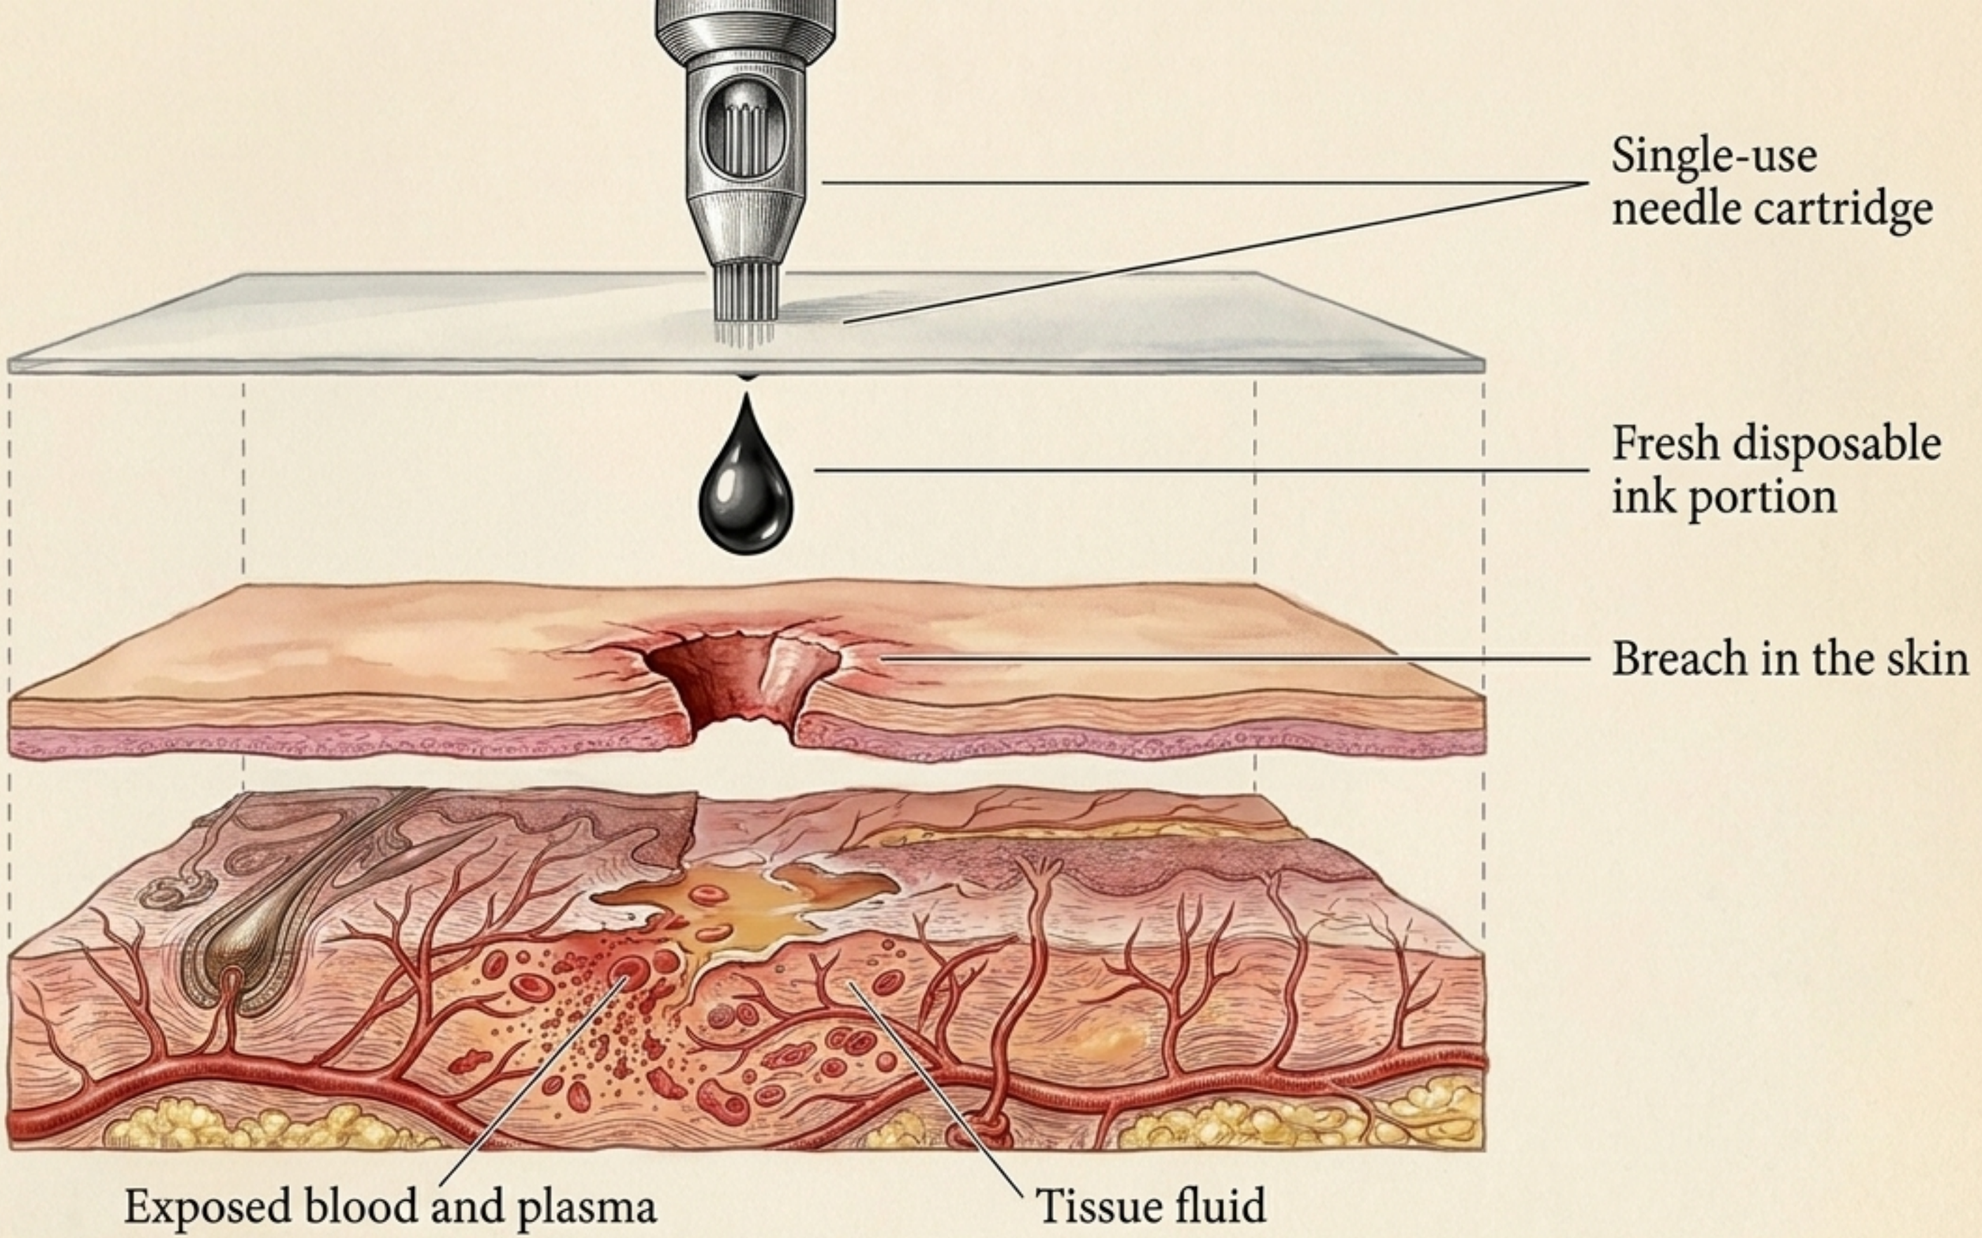


Safe procedure demands absolute separation between contaminated surfaces and sterile equipment layers.

VERIFY THE CONTROLLED PROCESS