
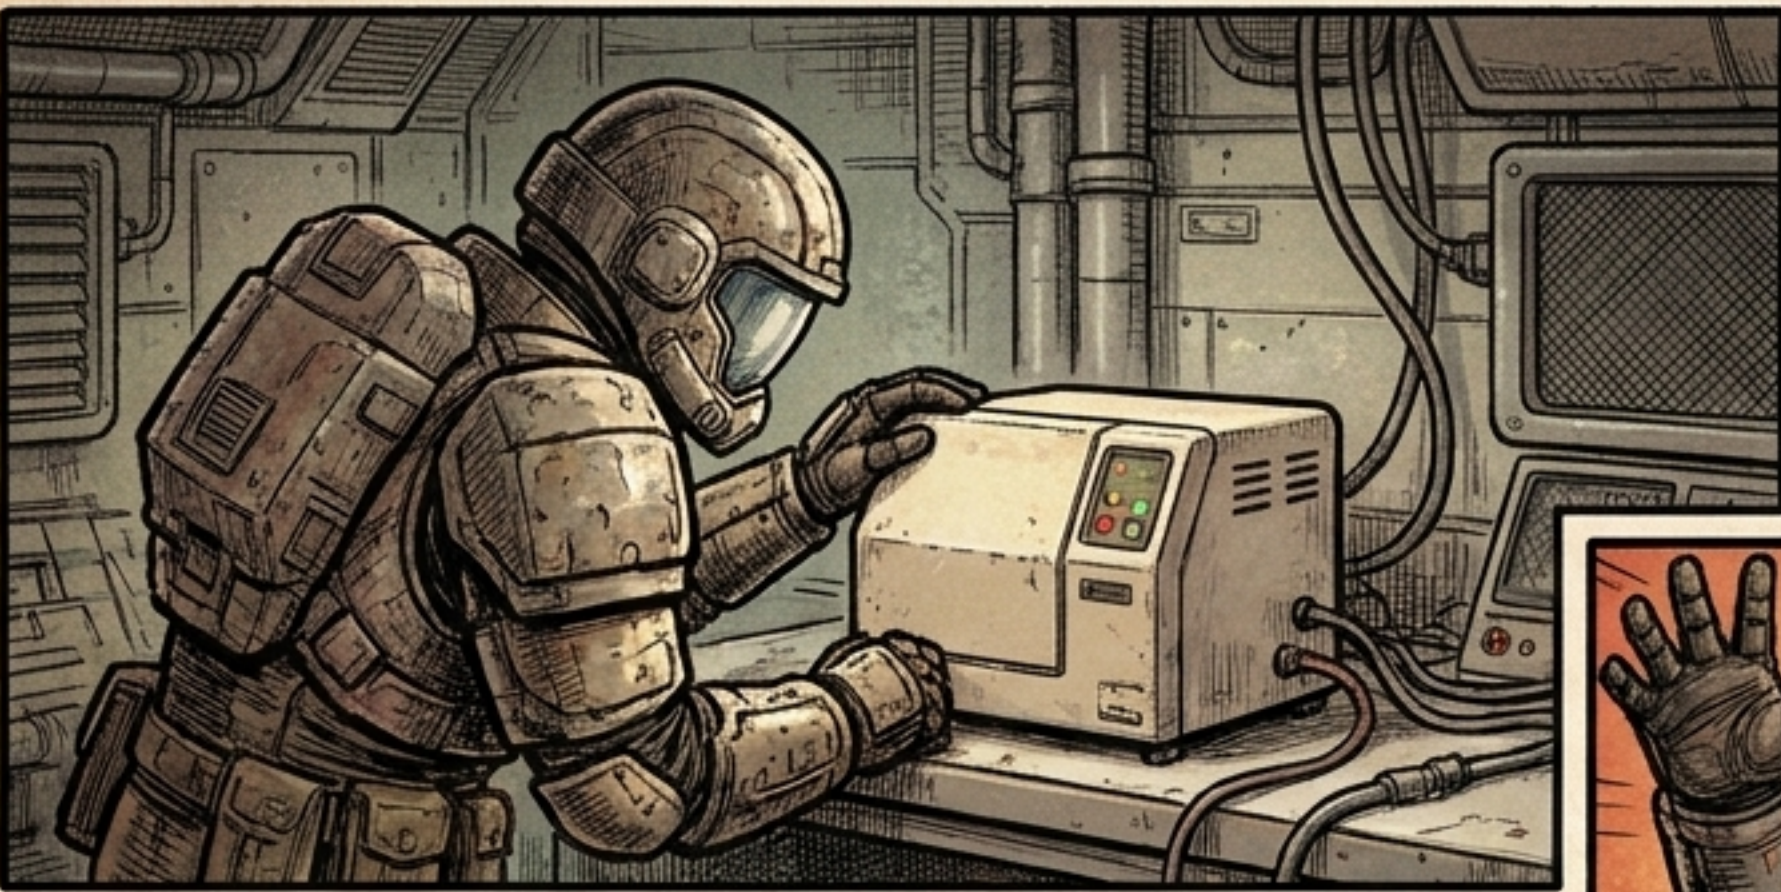


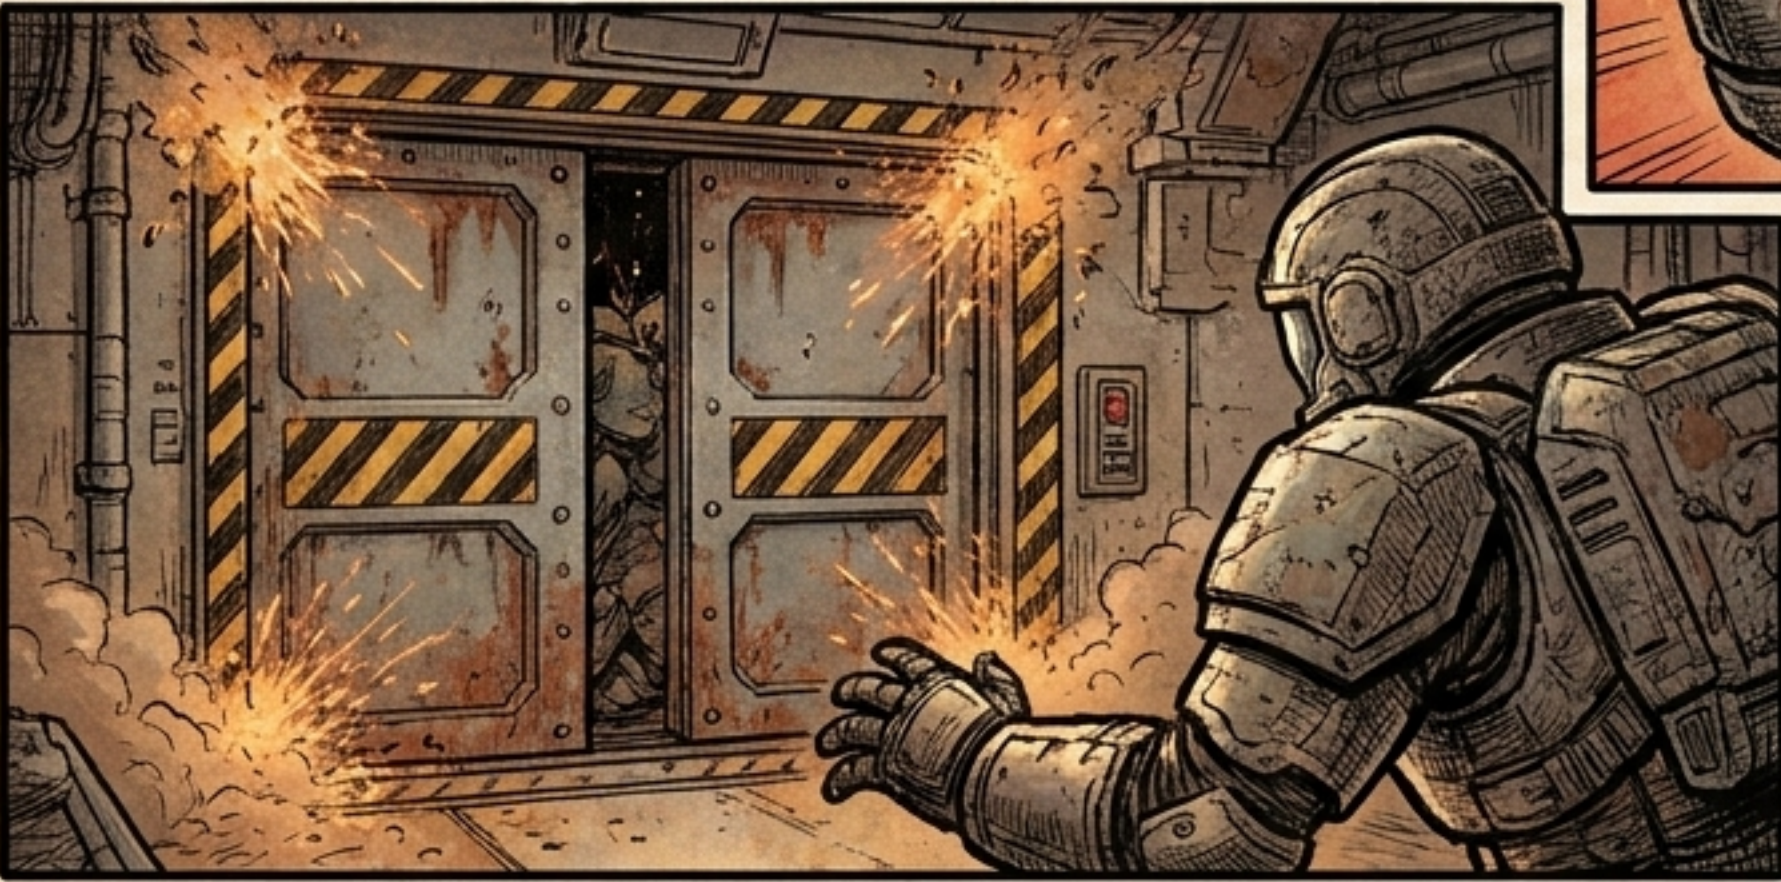

**"A failed sterilization indicator is evidence that the process needs investigation before instruments return to service."
"Initiating planetary lockdown might be a slight overreaction to a damp pouch."**