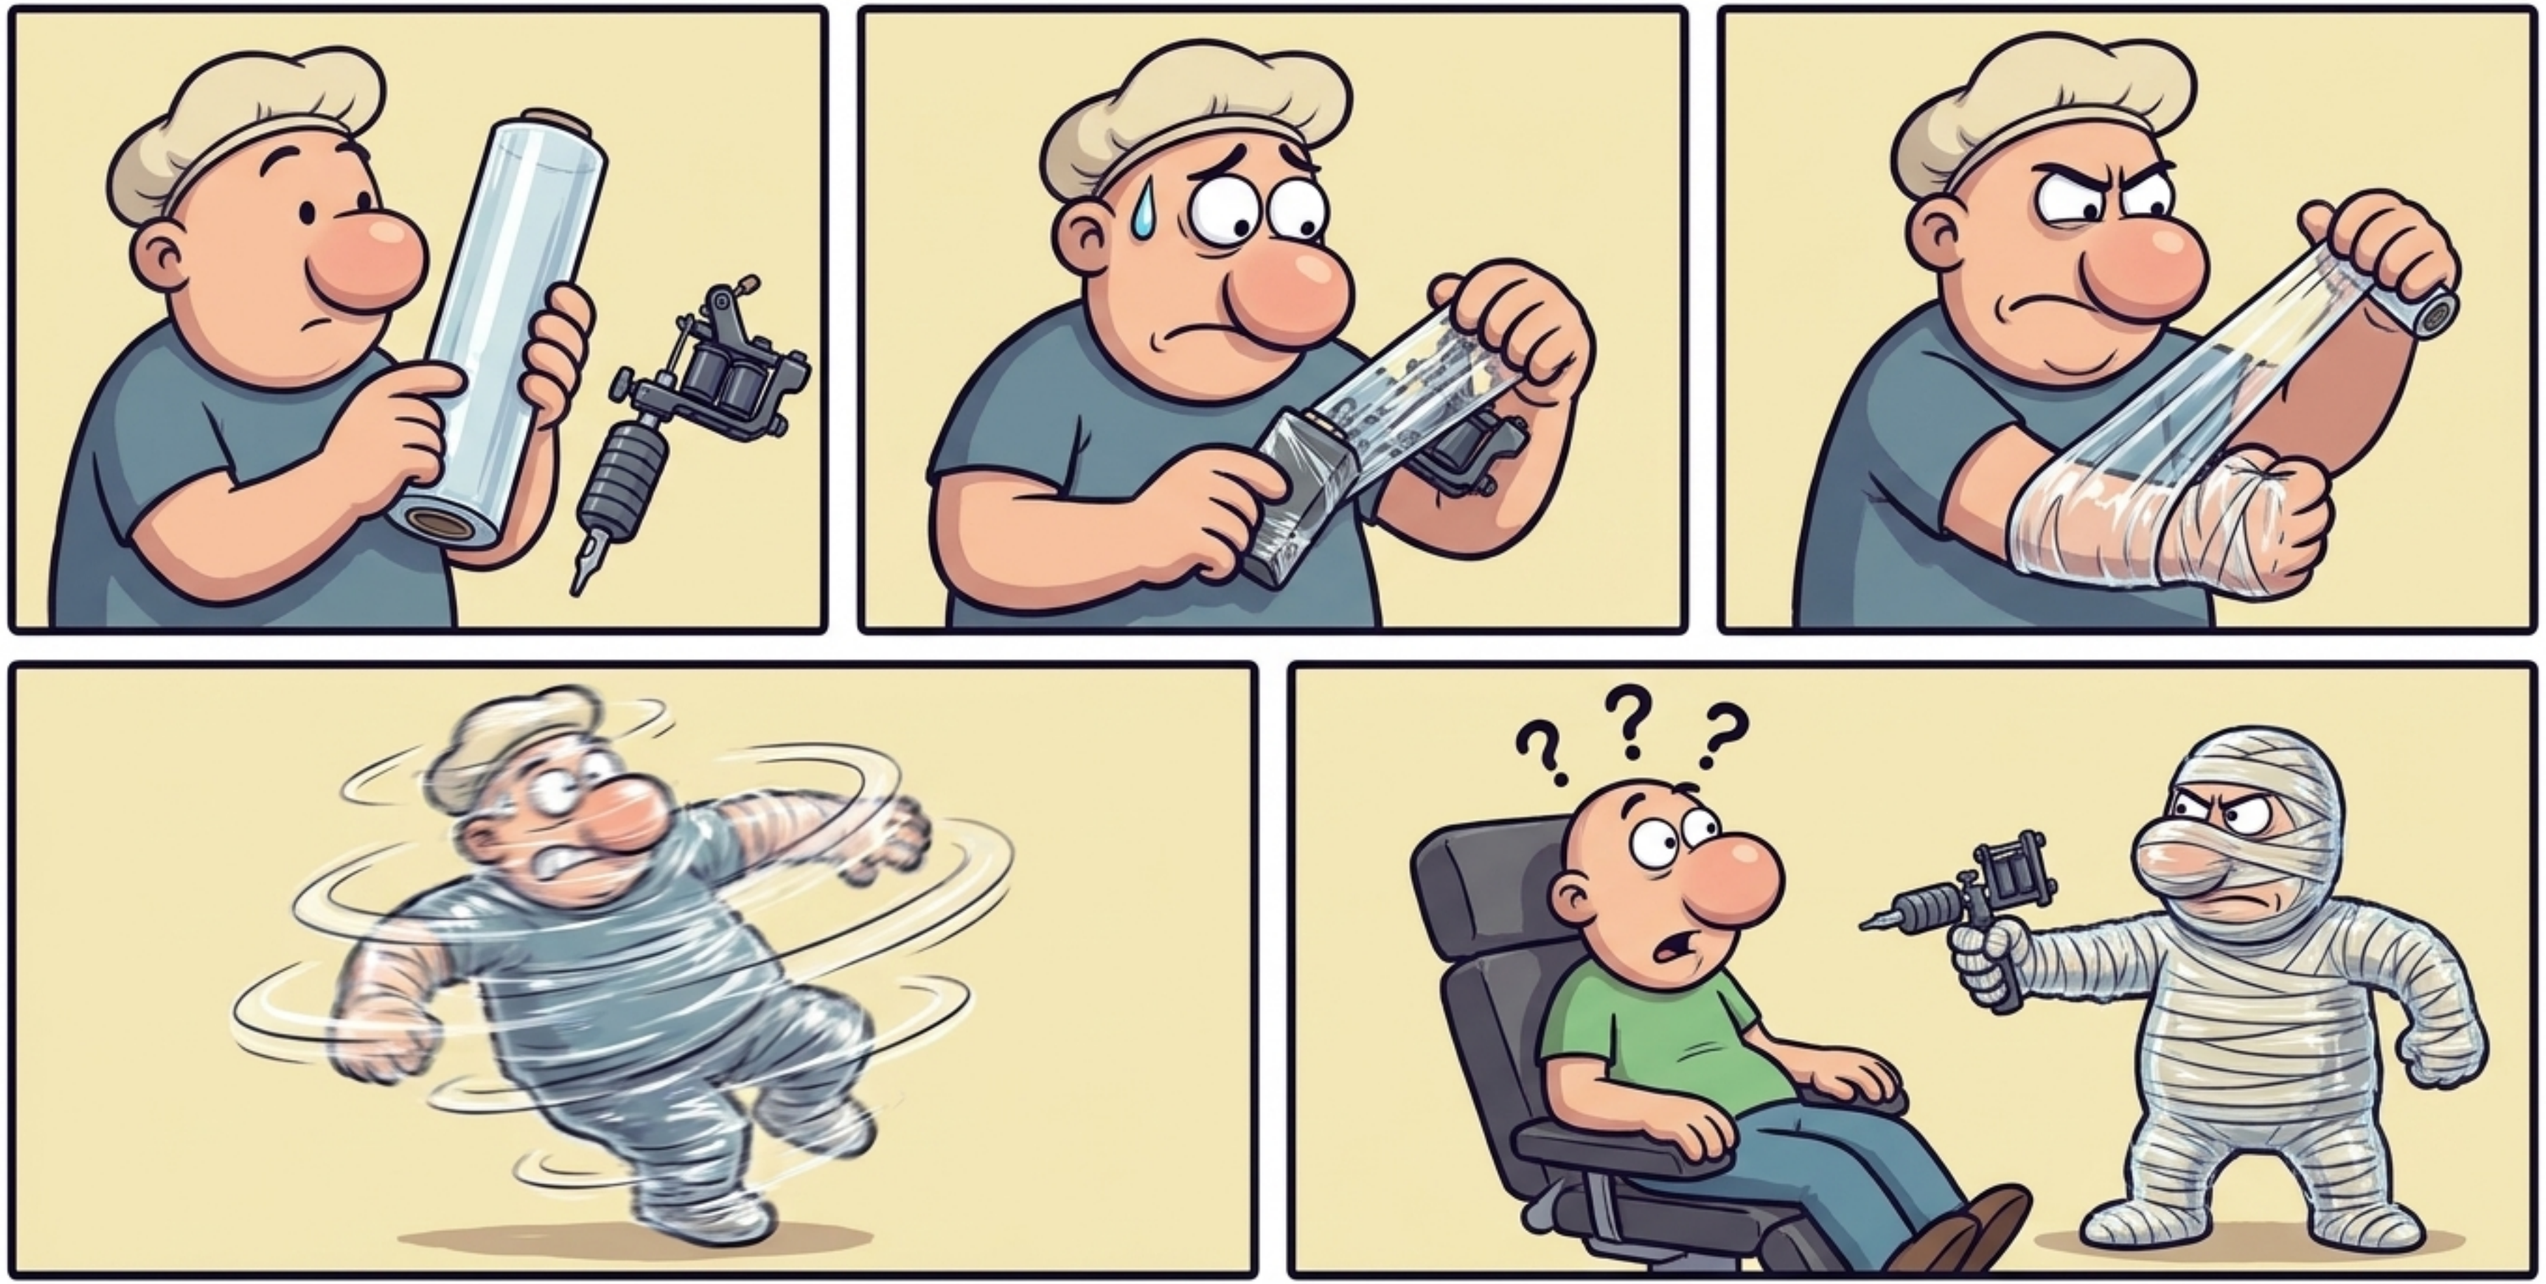


Every battery unit used clinically must be wrapped in disposable barrier film covering all exposed surfaces. Mummification is a valid infection control strategy.